

M.I.K. Santala

Custom Silicon Detectors to Enhance JET Neutral Particle Analysers for DT Operations

(14th April – 17th April 2015)
Frascati, Italy

“This document is intended for publication in the open literature. It is made available on the clear understanding that it may not be further circulated and extracts or references may not be published prior to publication of the original when applicable, or without the consent of the Publications Officer, EUROfusion Programme Management Unit, Culham Science Centre, Abingdon, Oxon, OX14 3DB, UK or e-mail Publications.Officer@euro-fusion.org”.

“Enquiries about Copyright and reproduction should be addressed to the Publications Officer, EUROfusion Programme Management Unit, Culham Science Centre, Abingdon, Oxon, OX14 3DB, UK or e-mail Publications.Officer@euro-fusion.org”.

The contents of this preprint and all other EUROfusion Preprints, Reports and Conference Papers are available to view online free at <http://www.euro-fusionscipub.org>. This site has full search facilities and e-mail alert options. In the JET specific papers the diagrams contained within the PDFs on this site are hyperlinked.

Custom Silicon Detectors To Enhance Jet Neutral Particle Analysers For DT Operations

M. I. K. Santala^{*a,b,†}, J. Kalliopuska^c, N. Dzysiuk^{a,d}, P. Beaumont^{a,e}, A. Murari^{a,f}, R. R. E. Salomaa^{a,b}, and JET contributors^{%‡}

^aEUROfusion Consortium, JET, Culham Science Centre, Abingdon, OX14 3DB, UK

^bAalto University School of Science, Department of Applied Physics,
P.O. Box 14100, FI-00076 Aalto, Finland

^cAdvacam Ltd, Tietotie 3, 02150 Espoo, Finland

^dVR, Department of Physics and Astronomy, Uppsala University,
Box 516, SE-75120 Uppsala, Sweden

^eCCFE/Experiments Department, Culham Science Centre, Abingdon, OX14 3DB, UK

^fConsorzio RFX-Associazione EURATOM-ENEA per la Fusione, I-35127 Padova, Italy

E-mail: Marko.Santala@aalto.fi

JET neutral particle analysers (NPA) need to operate under demanding conditions. The main difficulty is the overlap between true ion signals and neutron-induced background. We have improved the background rejection dramatically by developing thin, custom silicon detectors optimised for ion detection on JET NPAs. The detectors have a silicon-on-insulator structure with the active layer ground to only a few microns but supported by a thick substrate to create a robust detector with an active thickness of 5 μm or 25 μm initially[1] and recently down to 3 μm . Although designed for JET, these detectors could find use in other fusion machines as well.

With the first batch of detectors, the JET high energy NPA has been upgraded and its performance demonstrated in high-power DD campaigns. With 5 μm detectors, there is essentially no overlap between ion signals and background, and with 25 μm detectors the signal and background are better separated due to improved pulse-height response. With the second batch, the aim is to upgrade also the low-energy NPA. We will also discuss MCNP results on the anticipated performance in DT conditions.

*1st EPS conference on Plasma Diagnostics
14-17 April 2015
Frascati, Italy*

*Speaker.

†Corresponding author.

‡% See the Appendix of F. Romanelli et al., Proceedings of the 25th IAEA Fusion Energy Conference 2014, Saint Petersburg, Russia

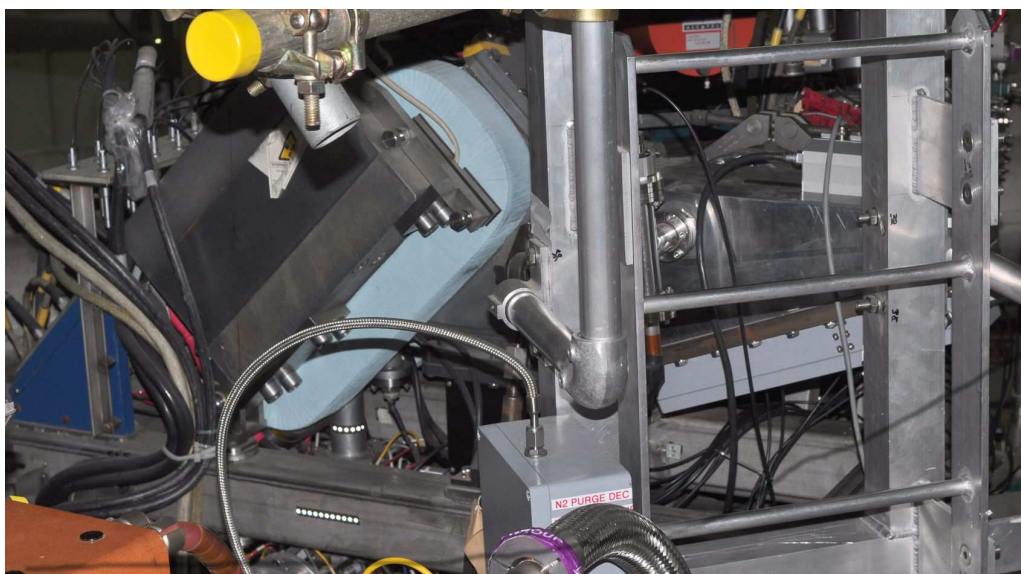


Figure 1: JET high energy NPA KF1. Neutral atoms enter the diagnostic along vertical beamline, are ionised by a thin carbon foil (not visible), bent through 90° by electromagnet (blue coil) and off the plane by electrostatic plates before entering the detector chamber (wedge-like part). Detectors are lined along the sloped edge of the chamber and connected directly to electronics (gray box).

1. JET neutral particle analysers

Neutral particle analysers are unique diagnostics because they are the only diagnostics capable of measuring plasma ions deep in plasma. In principle, their operation is simple: some of the plasma ions are first neutralised in plasma, releasing them from the magnetic confinement, and these neutrals are measured after escaping the plasma. However, the analysis of neutralisation and reionisation are often challenging problems on their own. The measured signals are integrals along the line-of-sight through entire plasma.

JET has two neutral particle analysers (NPA): the high-energy NPA (KF1, Fig. 1) has a vertical line-of-sight through plasma core. It is predominantly used for measuring fusion products and RF-accelerated ions. For hydrogenous ions it can operate typically from 250 keV to 1-1.5 MeV and up to 3 MeV for helium ions. The low-energy NPA (KR2) has a horizontal, radial line-of-sight through the plasma core. It can be configured for various energy ranges starting from 5 keV up to 750 keV for hydrogen. It is ultimately intended for the measurement of plasma isotope composition profile, however, achieving this has proven rather difficult due to highly non-thermal ion population present in typical JET plasmas.

Both JET NPAs have similar operating principle: neutrals escaping the plasma are first reionised by a thin carbon foil (40 nm), then dispersed spatially first in momentum by a electromagnet followed by a transverse deflection by electrostatic field separating different ion species. Ions are detected by a set of detectors arranged as a single row in KF1 and three rows in KR2. KF1 needs to be tuned to specific ion species whereas KR2 detects all hydrogenous species simultaneously. As ion species and energies are dispersed spatially, the ion detectors effectively only act as counters.

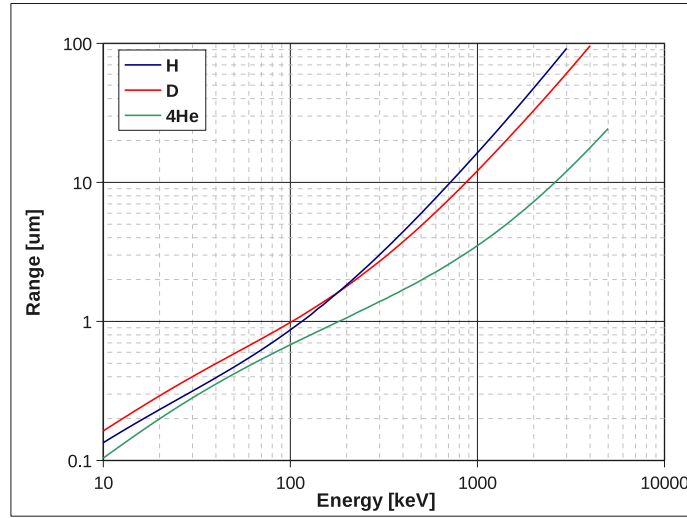


Figure 2: Range of hydrogenous and helium ions in Silicon, derived from tables in SRIM[3].

As there is generally little need for spectroscopy, detectors have so far been thin CsI(Tl) scintillators coupled to photomultipliers (PMTs), with highly nonlinear response. However, some spectroscopic performance is desired in practice. First, discrimination between ions and neutron-induced background is essential. Second, the electromagnetic dispersion is unable to separate ions with equal charge-to-mass (q/m) ratio, like deuterons and alphas. The ability to measure both separately is important for DT operations. The CsI(Tl) detectors also suffer from slow response ($3 \mu\text{s}$ decay constant) and PMT stability issues. These factors have led to the enhancement projects to develop custom Si detectors for the use in NPAs.

2. Custom silicon detectors

The use of silicon detectors for NPAs has been proposed long ago to improve the performance. However, commercially available detectors are typically much thicker (order of $100 \mu\text{m}$) than the ion ranges at the relevant energies (Figure 2). At the typical energies, the necessary detector thickness is only a few μm . The excess detector volume is only harmful by detecting background and increasing the effects of radiation damage, another problem with commercial detectors.

The issues with commercial detectors and access to semiconductor fabrication facilities at VTT/Aalto Micronova[2] led to the development of custom detectors aimed for JET NPAs with potential use of ITER also kept in mind. To match the ion range with the active detector volume while producing mechanically robust detectors, Silicon-on-Insulator (SOI) structure was chosen (Figure 3). These are manufactured by bonding a high-resistivity p-type active wafer to technical grade substrate wafer and grinding the active wafer to desired thickness. In the initial batch[1], detectors with active thickness of $5 \mu\text{m}$ and $25 \mu\text{m}$ were made, the former at the limit-of-technology and the latter close to the range of highest energy protons.

Internally, the detectors are split into strips which act as independent sub-detectors. In the initial batch, the active area was 7 by 10 mm in 64 strips ($110 \mu\text{m}$ pitch). The strips are insulated

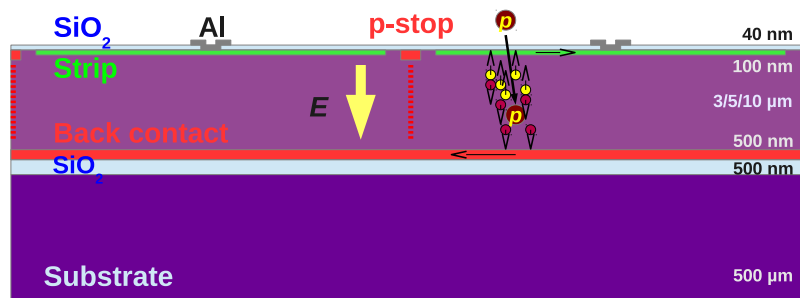


Figure 3: Schematic structure of the SOI thin ion detectors.

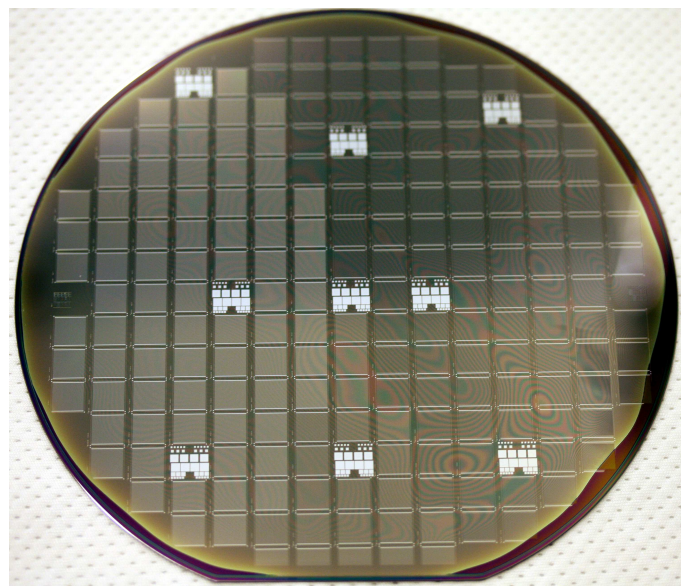


Figure 4: Completed wafer of the recent batch. Note the interference fringes visible in the front of the wafer, these are caused by minute thickness variations of the top layer. In addition to detectors there are test structures at different radii.

from each other by a *p*-stop barrier which prevents charge from spreading into neighbouring strips. Splitting the detector into strips also helps to reduce capacitance and drastically reduces pile-up. If high capacitance and pile-up can be tolerated, strips can be read-out in parallel. In NPAs the strip structure is not needed for spectroscopic purposes. However, in other applications these detectors could likely be used as linear profilers for ions, low-energy X-rays or optical emissions.

In the second batch, just completed, the detector size has been changed to 7 by 7 mm in 32 strips (Figure 4). These are aimed for the low-energy NPA, so emphasis has been on making the top layer as thin as possible. In the new batch there are detectors with 3, 5, and 10 μm thickness.

3. High energy NPA upgrade

As the first step, the JET high energy NPA was upgraded with detectors from the initial batch.



Figure 5: A $5\ \mu\text{m}$ detector mounted on a PCB as installed on KF1 vacuum flange prior to installation on the machine. Hirose U-FL-series ultra-miniature connectors are used for bias (left) and AC-coupled signal connections (right). The detector is read-out as three banks of 20 strips. An IR LED for artificial excitation of the detectors is seen at lower left.

With only eight detectors in a simple linear arrangement this was seen as relatively simple process. Nevertheless, the entire data acquisition chain was redesigned at the same time. As silicon detectors have no intrinsic gain (unlike PMTs) much more sensitive preamplifiers were needed.

For the two lowest energy channels $5\ \mu\text{m}$ detectors were installed (see Fig. 5) and $25\ \mu\text{m}$ detectors were used for the remaining six channels. To reduce complexity, the thin detectors are read-out as three bundles of 20 strips and the thick ones as a single bundle. In total, there are 12 data acquisition channels. Each channel has a preamplifier, differential line driver, twisted-pair signal transmission from the machine to diagnostics hall, and a 14-bit 2 MS/s digitiser. The signal is digitised for the entire JET pulse and ion events are located by numeric processing afterwards.

Sample pulse-height spectra of the new detectors during a high-power JET DD discharge are shown in 6. As there is no internal gain, pulse-height is proportional to energy. Hence, low-energy channel Ch1 has lowest typical pulse-height and the high-energy channel Ch8 the highest.

The thick detectors show an exponential component at low energies. This is caused by neutron-induced background, predominantly by Compton electrons and X-rays. Nevertheless, this component is well-separated from the ion signal apart from a slight overlap with Ch3. Hence, the radiation background has little impact on the analysis of the spectra.

Background rejection is even more remarkable with the thin detectors which show hardly any neutron-induced background at all. This improvement is far more than would be expected from the reduction of thickness alone because background mainly originates from particles which are not stopped by the active layer. Hence, background counts are not proportionate to active volume, but the pulse-height is roughly proportionate to thickness and the count-rate is likely independent of thickness. The thinner the detectors are, the easier it is to discriminate background from true ion events. With DT, the situation becomes more complex due to (n, p) and (n, α) reactions in silicon.

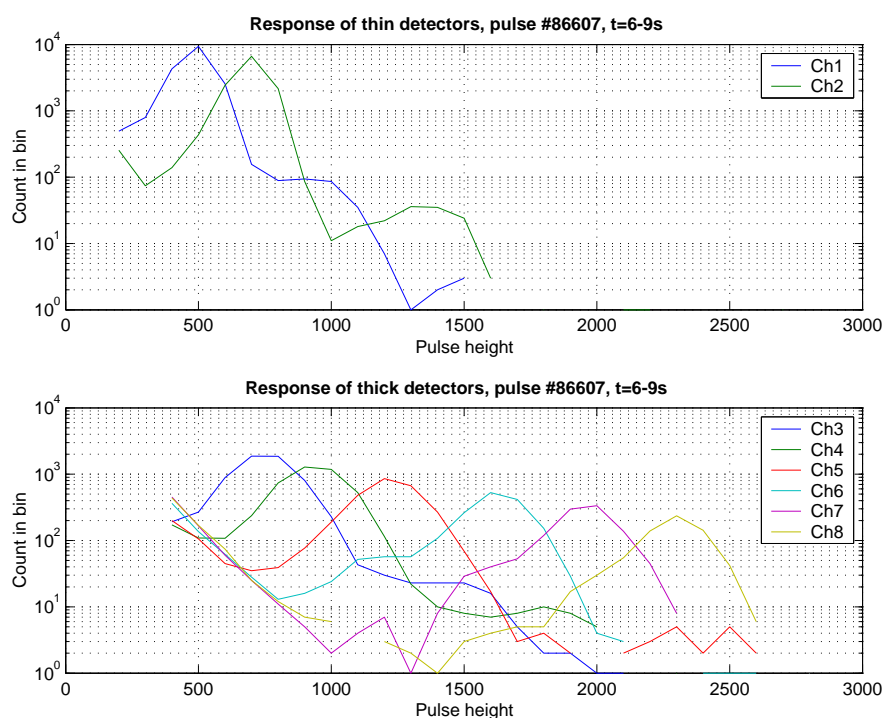


Figure 6: Time-integrated pulse-height-spectra of thin (top) and thick detectors of in JET pulse 86607 (binned data with bins of 50 ADC 'units', roughly 25 keV). At low pulse-heights, an exponential component caused by neutron-induced background is seen with thick detectors. Similar feature is nearly absent with thin detectors.

4. Low energy NPA upgrade

The excellent background rejection of the thin detectors in high energy NPA upgrade, was a decisive factor in launching the upgrade of low-energy NPA. This task is presently ongoing. The expected detector response has been modelled by MCNP, suggesting tolerable background even in full DT conditions. Due to much more refined mechanical structure, this upgrade is much more challenging than high-energy NPA. The readouts will also be implemented using complex multi-channel readout chips to avoid the high capacitance from paralleling many strips together.

Acknowledgments. This work has been carried out within the framework of the EUROfusion Consortium and has received funding from the Euratom research and training programme 2014-2018 under grant agreement No 633053. The views and opinions expressed herein do not necessarily reflect those of the European Commission.

References

- [1] J. Kalliopuska *et al.*, *A novel silicon detector for neutral particle analysis in JET fusion research*, Nucl. Inst. and Meth., Vol. **A591**, pages 92-97, (2008).
- [2] See <http://www.micronova.fi/>
- [3] *SRIM - The Stopping and Range of Ions in Matter* software available at <http://www.srim.org/>.